


Doppler Flow Pump

Model 769

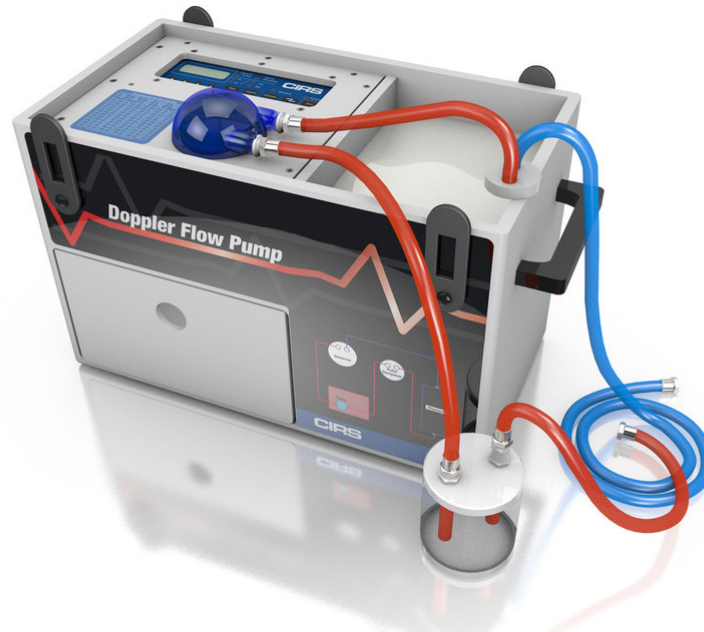

FLEXIBLE TESTING PLATFORM FOR DOPPLER ULTRASOUND

The Doppler Flow Pump is used to simulate blood flow when testing Doppler ultrasound devices. When used in conjunction with a tissue mimicking phantom (sold separately; a list of compatible CIRS phantoms is on the back), the flow pump supports routine Doppler quality assurance measurements of velocity accuracy, directional accuracy, sample volume accuracy and sensitivity. The configurable design also supports advanced research and engineering tests. For instance, test circuit may be modified to support either constant velocity flow or pulsatile flow. When in pulsatile flow mode, the peristaltic pump may be programmed to produce physiologic waveforms. In addition, the external tubing circuit ensures laminar flow rates over a wide range of flow rates, and it allows users to easily inject contrast agents for testing contrast enhanced ultrasound (CEUS).

The pump comes in a plastic ABS housing that conveniently stores all accessories needed for setting up a flow circuit, including:

- 1) A peristaltic pump that provides flow at rates from 0.04 to 750 ml/min, which translates to an average flow velocity of 2-70 cm/s. (Peak flow velocities will be 2-4 times greater than the average flow velocity, because of laminar and pulsatile flow.)
- 2) A fluid reservoir pre-filled with CIRS Doppler fluid. Replacement fluid may be ordered separately.
- 3) A pulse dampener that converts the pulsatile flow from the peristaltic pump into constant velocity flow.
- 4) Convenient color-coded tubing with quick-disconnect fittings
- 5) Graduated cylinder for purging phantoms of Doppler Fluid after each use. Also useful for calibrating the pump.
- 6) Pump-to-USB cable, allowing the pump to be programmed to mimic a human pulse. Instructions and examples are included.

Features

- Used in conjunction with ATS Urethane or Zerdine phantoms
- Max Flow Rate is 750 mL/ min
- Min Flow Rate can be as low as 0.04 mL/ min*
- Pulsatile or Constant Velocity configurations available
- Doppler fluid simulates acoustic and physical characteristics of blood
- All components stored in compact case for easy transport



*Actual value will vary depending on phantom used

900 Asbury Ave • Norfolk, Virginia 23513 • USA
Tel: 800.617.1177 • 757.855.2765 • Fax: 757.857.0523

WWW.CIRSINC.COM

CIRS

Tissue Simulation & Phantom Technology

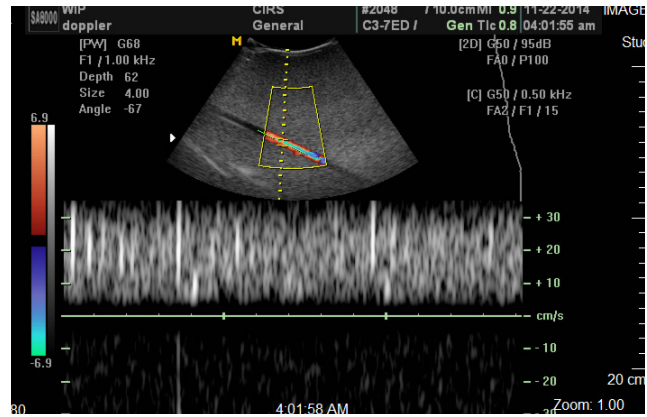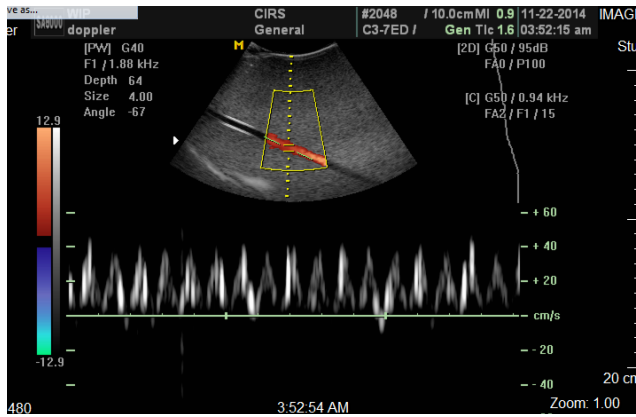

Doppler ultrasound images with Doppler Ultrasound Flow Phantom showing pulsatile and continuous flow.

SPECIFICATIONS

DOPPLER FLOW PUMP

| | |
|-------------------------|---|
| MOTOR TYPE | Step motor |
| MOTORSTEPSPERREVOLUTION | 200 |
| MICROSTEPPING | 1/8 to 1/1 depending on motor speed |
| DC CONNECTOR | 2.1mm, center positive |
| VOLTAGE AT DC CONNECTOR | 24V DC at full load |
| AMPERAGE | 900mA at full load |
| POWER SUPPLY TYPE | Unregulated linear external wall adapter, country and power source specific |
| POWERSUPPLYOUTPUTRATING | 24V DC @ 1A |
| DIMENSIONS | 9" x 4" x 8" High (23 cm x 10cm x 20 cm) |
| WEIGHT | 4.51 lbs. (2.05 kg) |
| MAXIMUM SPEED | 372 rpm |
| MINIMUM SPEED | 0.0168 rpm |
| MAXIMUM PUMPING RATE | 775.2 mL/min with 3/16 ID tubing |
| MINIMUM PUMPING RATE | 0.04 mL/min with 3/16 ID tubing |

DOPPLER FLUID (MODEL 769DF)

| PROPERTY | HUMAN BLOOD (37°C) | DOPPLER FLUID (22°C) |
|--|---------------------|----------------------|
| Viscosity (mPa) | 3 | 4 ± 0.5 |
| Velocity (m/s) | 1583 | 1570 ± 30 |
| Attenuation (dB/cm/MHz) | 0.15 | < 0.1 |
| Backscatter (f ⁴ m ⁻¹ sr ⁻¹) | 4x10 ⁻³¹ | Not Measured |
| Fluid Properties | Non Newtonian | Newtonian |

"Validation of a New Blood-Mimicking Fluid for Use in Doppler Flow Test Objects", K. Rammnarine, et. al., Ultrasound in Medicine & Biology, Vol. 24, No. 3, pp.454.

MODEL 769 INCLUDES

| QTY | COMPONENT DESCRIPTION |
|-----|---|
| 1 | Doppler Flow Pump* |
| 1 | Peristaltic Pump |
| 1 | Half Gallon of CIRS Doppler fluid (769DF) |
| 1 | Pulse dampener |
| 1 | Tubing Pack |
| 1 | Graduated Cylinder |
| 1 | Set of two Control Cables |
| - | 24-Month Warranty |
| - | User Guide |

*Local power supply adapters not included.

COMPATIBLE PHANTOMS*

| MODEL | DESCRIPTION |
|----------------|---|
| ATS 524 & 525 | Peripheral Vascular Doppler Flow Phantom |
| ATS 527 | Doppler Flow Directional Discrimination Phantom |
| ATS 523 & 523A | Cardiac Doppler Flow Phantom |
| 069A | Doppler Flow Phantom |

*Must be purchased separately

Custom phantoms are available upon request. Contact customer service at admin@cirsinc.com for more information.

